

Human SIRPG ELISA Kit

Sandwich ELISA

Catalog EL-213-192

INTRODUCTION

SIRPG encodes signal-regulatory protein gamma (SIRP-gamma), an immunoglobulin superfamily member closely related to SIRPA, expressed primarily on the surface of T lymphocytes. Structural and functional studies indicate that SIRP-gamma binds the widely distributed protein CD47 on antigen-presenting cells, and this interaction supports integrin-independent adhesion between the two cell types while delivering a costimulatory boost to T-cell receptor signaling, increasing antigen-driven T-cell proliferation. This stimulatory role sets SIRPG apart from its inhibitory paralog SIRPA, since SIRP-gamma lacks the cytoplasmic signaling motifs that let SIRPA recruit inhibitory phosphatases; general reference summaries describing the SIRP family as inhibitory regulators of tyrosine-kinase signaling appear to reflect that broader family pattern rather than SIRPG's own, largely costimulatory function. Alternative splicing of the gene is known to generate additional protein isoforms, though their individual functional consequences remain less well defined.

PRINCIPLE OF THE ASSAY

This kit uses a sandwich enzyme immunoassay format to detect Human SIRPG. Microtiter plate wells are pre-coated with a SIRPG-specific capture antibody that binds the target analyte present in standards or samples. A biotin-conjugated detection antibody, also specific to Human SIRPG, is then added to each well, followed by incubation with Avidin conjugated to horseradish peroxidase (HRP). Color development occurs only in wells where Human SIRPG, the biotin-conjugated detection antibody, and the Avidin-HRP conjugate are all present, upon addition of TMB substrate solution. The enzymatic reaction is stopped by the addition of sulphuric acid solution, and the resulting color change is measured spectrophotometrically at 450 nm (± 10 nm). Sample concentrations are determined by comparing well absorbance values against a standard curve.

MATERIALS AND STORAGE

Store kit components at -20°C unless specified otherwise. DO NOT USE past kit expiration date. Some vials contain a small amount of reagents. Spin tubes on pulse setting prior to opening.

Each kit includes:	Units
Pre-Coated Microplate	12 strips x 8 wells
Standard (Lyophilized)	2 vials
Biotinylated Antibody (100 $\times$)	120 μL
Streptavidin-HRP (100 $\times$)	120 μL
Standard/Sample Diluent Buffer	20 mL
Biotinylated Antibody Diluent	12 mL
HRP Diluent	12 mL
Wash Buffer (25 $\times$)	20 mL
TMB Substrate Solution	10 mL
Stop Reagent	6 mL
Plate Covers	2 pieces
<i>Do not mix or substitute reagents with those from other lots.</i>	

MATERIALS AND INSTRUMENTS REQUIRED BUT NOT SUPPLIED

- Precision pipettes calibrated to deliver 5-1000 μL
- Multi-channel pipette calibrated to deliver 50-200 μL
- Plate shaker
- Disposable tips
- Vortex-Mixer
- Distilled or de-ionized water
- Microplate reader capable of reading 450nm with background subtraction at 620nm

SAFETY PRECAUTIONS

- The test protocol must be followed strictly.
- All reagents containing human material should be handled as if potentially infectious. Operators should wear gloves and protective

clothing when handling any patient sera or serum based products.

- The kit reagents contain antimicrobial agents, acid and 3,3',5,5'-tetramethylbenzidine. Avoid contact with the skin and eyes. Rinse immediately with plenty of water if any contact occurs.
- Any liquid that has been brought into contact with potentially infectious material has to be discarded in a container with a disinfectant. Disposal must be performed in accordance with local regulations.
- Disposal must be performed in accordance with local regulations.
- Only trained laboratory personnel should execute this test.

Human SIRPG ELISA Kit

Sandwich ELISA

Catalog EL-213-192

PREPARATION OF REAGENTS

Prepare only the appropriate amount of required reagent on the day of use. Store all reagents as per instructions stated on the label.

- 1. Wash Buffer (1X) Preparation: Dilute the 25X wash buffer concentrate 1:25 with double-distilled Water.**
- 2. Detection Reagent (1X) Preparation: Dilute the biotinylated antibody and streptavidin-HRP concentrates 100-fold with Biotinylated Antibody Diluent and HRP Diluent, respectively, immediately before use.**
- 3. Preparation of Calibrators: Prepare calibrators by serial dilution from a 10 down to 0.16 (plus a 0 blank), per the source manual.**

Sol'n ID	Source	Source Vol (µL)	Cal. Diluent (µL)	Final Vol (µL)	Final Conc. (ng/mL)
Std 1	Stock Standard	500	500	1000	10
Std 2	Std 1	500	500	1000	5
Std 3	Std 2	500	500	1000	2.5
Std 4	Std 3	500	500	1000	1.25
Std 5	Std 4	500	500	1000	0.63
Std 6	Std 5	500	500	1000	0.32
Std 7	Std 6	500	500	1000	0.16
Blank	Std 7	500	500	1000	0

SPECIMEN STORAGE

This kit is compatible with EDTA-plasma, heparin-plasma and serum samples. Samples can be stored at or below -20°C for up to 1 year.

ASSAY PROCEDURE

1. After the kit is equilibrated at room temperature, add 100 µL of Standard Working Buffer (gradually diluted according to the instructions) or 100 µL of sample to each well, and incubate at 37°C for 80 minutes.
2. Discard the liquid in the plate, add 200 µL 1× Wash Buffer to each well, and wash the plate 3 times. After pat it dry against clean absorbent paper, add 100 µL Biotinylated Antibody Working Solution (1×) to each well, incubate at 37°C for 50 minutes.
3. Discard the liquid in the plate, add 200 µL 1× Wash Buffer to each well, and wash the plate 3 times. After pat it dry against clean absorbent paper, add 100 µL 1× Streptavidin-HRP Working Solution to each well, incubate at 37°C for 50 minutes.
4. Discard the liquid in the plate, add 200 µL 1× Wash Buffer to each well, and wash the plate 5 times. After pat it dry against clean absorbent paper, add 90 µL TMB Substrate Solution to each well, incubate at 37°C for 20 minutes in the dark.
5. Add 50 µL Stop Solution to each well, shake plate on a plate shaker for 1 minute to mix. Record the OD at 450 nm immediately, calculation of the results.

CALCULATIONS AND RESULTS

1. Construct a standard curve by plotting the absorbance obtained from each standard against concentration. Use a 4 or 5 parameter curve fit. Alternatively a log-log curve fit may be used.
2. The concentration of the unknowns can be read directly from this standard curve using the absorbance value for each sample.

3. Any sample undiluted or diluted still reading greater than the highest standard should be diluted appropriately and retested. If the samples have been diluted, the concentration determined from the standard curve must be multiplied by the dilution factor.

PERFORMANCE CHARACTERISTICS

Precision: Intra-assay CV < 8%. Inter-assay CV < 10%.


Detection Limit: 0.064 ng/mL

Recovery: Serum (n = 5): 83-95% (avg 89%); EDTA plasma (n = 5): 87-97% (avg 90%); Heparin plasma (n = 5): 81-95% (avg 88%)

Specificity: This assay has high sensitivity and excellent specificity for detection of Human SIRP α . No significant cross-reactivity or interference between Human SIRP α and analogues was observed.

Human SIRPG ELISA Kit Sandwich ELISA Catalog EL-213-192

SAMPLE STANDARD CURVE

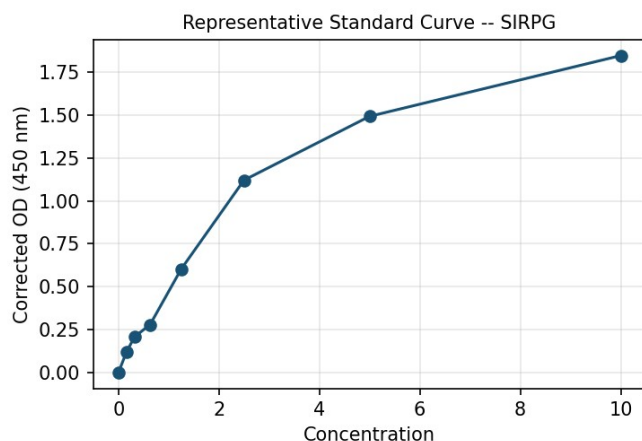

Representative standard curve shown for illustration only. This curve should not be used to calculate unknown sample concentrations -- run a new standard curve with each assay.

ORDERING INFORMATION

Please visit www.affinityimmuno.com to order this product. Visa, Mastercard, AMEX and PayPal are accepted in our online store.

Your order will be processed immediately and you will be notified with a delivery timeframe.