

Human CD133/PROM1 ELISA Kit

Sandwich ELISA

Catalog EL-213-34133

INTRODUCTION

PROM1 encodes CD133, a five-transmembrane-domain glycoprotein that localizes to cholesterol-rich microdomains within membrane protrusions and helps organize the apical surface of polarized epithelial cells. It is widely used as a marker of stem and progenitor populations, including hematopoietic and neural stem cells, and of stem-like subpopulations within several tumor types, where it appears to help maintain an undifferentiated state by engaging PI3K/Akt, MAPK/ERK, Wnt, and TGF-beta signaling networks. During eye development CD133 plays a specific role in shaping photoreceptor outer-segment discs, and inherited mutations that disrupt this function underlie a spectrum of retinal degenerations, including forms of retinitis pigmentosa, cone-rod dystrophy, Stargardt disease, and macular dystrophy. Regulation of the gene through several tissue-specific promoters allows this single protein to serve distinct purposes across stem cell biology, cancer, and retinal physiology.

PRINCIPLE OF THE ASSAY

This kit uses a sandwich enzyme immunoassay format to measure human CD133/PROM1. Wells of the microtiter plate are pre-coated with a capture antibody specific to human PROM1, which binds the target analyte present in standards or samples. A biotin-conjugated detection antibody, also specific to human PROM1, is then added and binds a distinct epitope on the captured analyte. Avidin conjugated to horseradish peroxidase (HRP) is subsequently introduced and binds the biotin moiety, completing the detection complex. Upon addition of TMB substrate solution, a colorimetric signal develops only in wells where human PROM1, the biotin-conjugated detection antibody, and avidin-HRP are all present. The enzymatic reaction is stopped by the addition of a sulphuric acid stop solution, and absorbance is read at 450 nm (± 10 nm). PROM1 concentrations in the samples are then determined by referencing the measured optical densities against a standard curve.

MATERIALS AND STORAGE

Store kit components at -20°C unless specified otherwise. DO NOT USE past kit expiration date. Some vials contain a small amount of reagents. Spin tubes on pulse setting prior to opening.

Each kit includes:	Units
Pre-Coated Microplate	12 strips x 8 wells
Standard (Lyophilized)	2 vials
Biotinylated Antibody (100 $\times$)	120 μL
Streptavidin-HRP (100 $\times$)	120 μL
Standard/Sample Diluent Buffer	20 mL
Biotinylated Antibody Diluent	12 mL
HRP Diluent	12 mL
Wash Buffer (25 $\times$)	20 mL
TMB Substrate Solution	10 mL
Stop Reagent	6 mL
Plate Covers	2 pieces

Do not mix or substitute reagents with those from other lots.

MATERIALS AND INSTRUMENTS REQUIRED BUT NOT SUPPLIED

- Precision pipettes calibrated to deliver 5-1000 μL
- Multi-channel pipette calibrated to deliver 50-200 μL
- Plate shaker
- Disposable tips
- Vortex-Mixer
- Distilled or de-ionized water
- Microplate reader capable of reading 450nm with background subtraction at 620nm

SAFETY PRECAUTIONS

- The test protocol must be followed strictly.
- All reagents containing human material should be handled as if potentially infectious. Operators

should wear gloves and protective clothing when handling any patient sera or serum based products.

- The kit reagents contain antimicrobial agents, acid and 3,3',5,5'-tetramethylbenzidine. Avoid contact with the skin and eyes. Rinse immediately with plenty of water if any contact occurs.
- Any liquid that has been brought into contact with potentially infectious material has to be discarded in a container with a disinfectant. Disposal must be performed in accordance with local regulations.
- Disposal must be performed in accordance with local regulations.
- Only trained laboratory personnel should execute this test.

Human CD133/PROM1 ELISA Kit

Sandwich ELISA

Catalog EL-213-34133

PREPARATION OF REAGENTS

Prepare only the appropriate amount of required reagent on the day of use. Store all reagents as per instructions stated on the label.

- 1. Wash Buffer (1X) Preparation: Dilute the 25X wash buffer concentrate 1:25 with double-distilled Water.**
- 2. Detection Reagent (1X) Preparation: Dilute the biotinylated antibody and streptavidin-HRP concentrates 100-fold with Biotinylated Antibody Diluent and HRP Diluent, respectively, immediately before use.**
- 3. Preparation of Calibrators: Prepare calibrators by serial dilution from a 10 down to 0.16 (plus a 0 blank), per the source manual.**

Sol'n ID	Source	Source Vol (μL)	Cal. Diluent (μL)	Final Vol (μL)	Final Conc. (ng/mL)
Std 1	Stock Standard	500	500	1000	10
Std 2	Std 1	500	500	1000	5
Std 3	Std 2	500	500	1000	2.5
Std 4	Std 3	500	500	1000	1.25
Std 5	Std 4	500	500	1000	0.63
Std 6	Std 5	500	500	1000	0.32
Std 7	Std 6	500	500	1000	0.16
Blank	Std 7	500	500	1000	0

SPECIMEN STORAGE

This kit is compatible with EDTA-plasma, heparin-plasma and serum samples. Samples can be stored at or below -20°C for up to 1 year.

ASSAY PROCEDURE

- After the kit is equilibrated at room temperature, add 100 μL of Standard Working Buffer (gradually diluted according to the instructions) or 100 μL of sample to each well, and incubate at 37°C for 80 minutes.
- Discard the liquid in the plate, add 200 μL 1× Wash Buffer to each well, and wash the plate 3 times. After pat it dry against clean absorbent paper, add 100 μL Biotinylated Antibody Working Solution (1×) to each well, incubate at 37°C for 50 minutes.
- Discard the liquid in the plate, add 200 μL 1× Wash Buffer to each well, and wash the plate 3 times. After pat it dry against clean absorbent paper, add 100 μL 1× Streptavidin-HRP Working Solution to each well, incubate at 37°C for 50 minutes.
- Discard the liquid in the plate, add 200 μL 1× Wash Buffer to each well, and wash the plate 5 times. After pat it dry against clean absorbent paper, add 90 μL TMB Substrate Solution to each well, incubate at 37°C for 20 minutes in the dark.
- Add 50 μL Stop Solution to each well, shake plate on a plate shaker for 1 minute to mix. Record the OD at 450 nm immediately, calculation of the results.

CALCULATIONS AND RESULTS

- Construct a standard curve by plotting the absorbance obtained from each standard against concentration. Use a 4 or 5 parameter curve fit. Alternatively a log-log curve fit may be used.
- The concentration of the unknowns can be read directly from this standard curve using the absorbance value for each

sample.

3. Any sample undiluted or diluted still reading greater than the highest standard should be diluted appropriately and retested. If the samples have been diluted, the concentration determined from the standard curve must be multiplied by the dilution factor.

PERFORMANCE CHARACTERISTICS

Precision: Intra-assay CV < 8%. Inter-assay CV < 10%.

Detection Limit: 0.054 ng/mL

Recovery: Serum (n = 5): 80-97% (avg 88%); EDTA plasma (n = 5): 83-95% (avg 89%); Heparin plasma (n = 5): 90-105% (avg 97%)

Specificity: This assay has high sensitivity and excellent specificity for detection of Human PROM1. No significant cross-reactivity or interference between Human PROM1 and analogues was observed.




This kit employs a sandwich enzyme immunoassay technique to quantify human CD133/PROM1 in biological samples.

Human CD133/PROM1 ELISA Kit

Sandwich ELISA

Catalog EL-213-34133

SAMPLE STANDARD CURVE

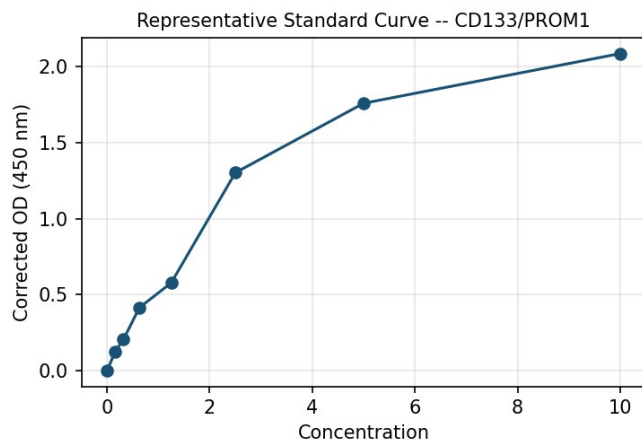

Representative standard curve shown for illustration only. This curve should not be used to calculate unknown sample concentrations -- run a new standard curve with each assay.

ORDERING INFORMATION

Please visit www.affinityimmuno.com to order this product. Visa, Mastercard, AMEX and PayPal are accepted in our online store.

Your order will be processed immediately and you will be notified with a delivery timeframe.