

Human CD155 ELISA Kit

Sandwich ELISA

Catalog EL-213-34155

INTRODUCTION

PVR, better known by its surface designation CD155, is a single-pass membrane glycoprotein of the immunoglobulin superfamily that normally helps glue epithelial cells together at adherens junctions and lets cells grip the surrounding matrix through vitronectin. On immune cells it does double duty as a ligand: it engages the activating receptor CD226 and the inhibitory receptors TIGIT and CD96 on natural killer and T cells, and this competitive three-way interaction shapes whether those cells become cytotoxic or stand down, forming a stable contact point called the immunological synapse in the process. Many solid tumors upregulate CD155, which appears to help them dodge immune surveillance and can also promote tumor cell movement and invasion directly. The molecule is also historically notable as the entry point that poliovirus, and separately pseudorabies virus, use to infect human cells, a property confined to primates that gave the gene its original name.

PRINCIPLE OF THE ASSAY

This kit utilizes a sandwich enzyme immunoassay format in which the microtiter plate wells are pre-coated with a capture antibody specific to human CD155 (PVR). During the assay, standards or samples are introduced into the appropriate wells along with a biotin-conjugated detection antibody that also recognizes human CD155. Avidin conjugated to horseradish peroxidase (HRP) is then added to each well and allowed to incubate, linking the enzymatic reporter to the captured analyte via the biotin-avidin interaction. Upon addition of TMB substrate solution, a colorimetric signal develops exclusively in wells containing human CD155, biotin-conjugated antibody, and avidin-HRP. The enzymatic reaction is stopped by the addition of a sulphuric acid stop solution, and the resulting color change is measured spectrophotometrically at 450 nm (± 10 nm). Sample concentrations are determined by comparing the optical density readings of each sample against a reference standard curve.

MATERIALS AND STORAGE

Store kit components at -20°C unless specified otherwise. DO NOT USE past kit expiration date. Some vials contain a small amount of reagents. Spin tubes on pulse setting prior to opening.

Each kit includes:	Units
Pre-Coated Microplate	12 strips x 8 wells
Standard (Lyophilized)	2 vials
Biotinylated Antibody (100 $\times$)	120 μL
Streptavidin-HRP (100 $\times$)	120 μL
Standard/Sample Diluent Buffer	20 mL
Biotinylated Antibody Diluent	12 mL
HRP Diluent	12 mL
Wash Buffer (25 $\times$)	20 mL
TMB Substrate Solution	10 mL
Stop Reagent	6 mL
Plate Covers	2 pieces
<i>Do not mix or substitute reagents with those from other lots.</i>	

MATERIALS AND INSTRUMENTS REQUIRED BUT NOT SUPPLIED

- Precision pipettes calibrated to deliver 5-1000 μL
- Multi-channel pipette calibrated to deliver 50-200 μL
- Plate shaker
- Disposable tips
- Vortex-Mixer
- Distilled or de-ionized water
- Microplate reader capable of reading 450nm with background subtraction at 620nm

SAFETY PRECAUTIONS

- The test protocol must be followed strictly.
- All reagents containing human material should be handled as if potentially infectious. Operators should wear gloves and protective

clothing when handling any patient sera or serum based products.

- The kit reagents contain antimicrobial agents, acid and 3,3',5,5'-tetramethylbenzidine. Avoid contact with the skin and eyes. Rinse immediately with plenty of water if any contact occurs.
- Any liquid that has been brought into contact with potentially infectious material has to be discarded in a container with a disinfectant. Disposal must be performed in accordance with local regulations.
- Disposal must be performed in accordance with local regulations.
- Only trained laboratory personnel should execute this test.

Human CD155 ELISA Kit

Sandwich ELISA

Catalog EL-213-34155

PREPARATION OF REAGENTS

Prepare only the appropriate amount of required reagent on the day of use. Store all reagents as per instructions stated on the label.

- 1. Wash Buffer (1X) Preparation: Dilute the 25X wash buffer concentrate 1:25 with double-distilled Water.**
- 2. Detection Reagent (1X) Preparation: Dilute the biotinylated antibody and streptavidin-HRP concentrates 100-fold with Biotinylated Antibody Diluent and HRP Diluent, respectively, immediately before use.**
- 3. Preparation of Calibrators: Prepare calibrators by serial dilution from a 1000 down to 15.63 (plus a 0 blank), per the source manual.**

Sol'n ID	Source	Source Vol (μL)	Cal. Diluent (μL)	Final Vol (μL)	Final Conc. (ng/mL)
Std 1	Stock Standard	500	500	1000	1000
Std 2	Std 1	500	500	1000	500
Std 3	Std 2	500	500	1000	250
Std 4	Std 3	500	500	1000	125
Std 5	Std 4	500	500	1000	62.5
Std 6	Std 5	500	500	1000	31.25
Std 7	Std 6	500	500	1000	15.63
Blank	Std 7	500	500	1000	0

SPECIMEN STORAGE

This kit is compatible with EDTA-plasma, heparin-plasma and serum samples. Samples can be stored at or below -20°C for up to 1 year.

ASSAY PROCEDURE

1. After the kit is equilibrated at room temperature, add 100 μL of Standard Working Buffer (gradually diluted according to the instructions) or 100 μL of sample to each well, and incubate at 37°C for 80 minutes.
2. Discard the liquid in the plate, add 200 μL 1× Wash Buffer to each well, and wash the plate 3 times. After pat it dry against clean absorbent paper, add 100 μL Biotinylated Antibody Working Solution (1×) to each well, incubate at 37°C for 50 minutes.
3. Discard the liquid in the plate, add 200 μL 1× Wash Buffer to each well, and wash the plate 3 times. After pat it dry against clean absorbent paper, add 100 μL 1× Streptavidin-HRP Working Solution to each well, incubate at 37°C for 50 minutes.
4. Discard the liquid in the plate, add 200 μL 1× Wash Buffer to each well, and wash the plate 5 times. After pat it dry against clean absorbent paper, add 90 μL TMB Substrate Solution to each well, incubate at 37°C for 20 minutes in the dark.
5. Add 50 μL Stop Solution to each well, shake plate on a plate shaker for 1 minute to mix. Record the OD at 450 nm immediately, calculation of the results.

CALCULATIONS AND RESULTS

1. Construct a standard curve by plotting the absorbance obtained from each standard against concentration. Use a 4 or 5 parameter curve fit. Alternatively a log-log curve fit may be used.
2. The concentration of the unknowns can be read directly from this standard curve using the absorbance value for each sample.

3. Any sample undiluted or diluted still reading greater than the highest standard should be diluted appropriately and retested. If the samples have been diluted, the concentration determined from the standard curve must be multiplied by the dilution factor.

PERFORMANCE CHARACTERISTICS

Precision: Intra-assay CV < 8%. Inter-assay CV < 10%.

Detection Limit: 6 pg/mL

Recovery: Serum (n = 5): 78-95% (avg 86%); EDTA plasma (n = 5): 80-96% (avg 88%); Heparin plasma (n = 5): 80-92% (avg 86%)


Specificity: This assay has high sensitivity and excellent specificity for detection of Human PVR. No significant cross-reactivity or interference between Human PVR and analogues was observed.



This kit employs a sandwich enzyme immunoassay technique to quantify CD155 (PVR) in biological samples.

Human CD155 ELISA Kit Sandwich ELISA Catalog EL-213-34155

SAMPLE STANDARD CURVE

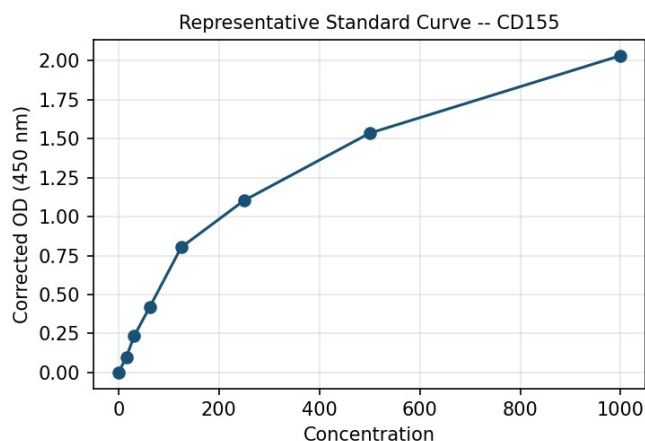

Representative standard curve shown for illustration only. This curve should not be used to calculate unknown sample concentrations -- run a new standard curve with each assay.

ORDERING INFORMATION

Please visit www.affinityimmuno.com to order this product. Visa, Mastercard, AMEX and PayPal are accepted in our online store.

Your order will be processed immediately and you will be notified with a delivery timeframe.