

Human IDO1 ELISA Kit

Sandwich ELISA

Catalog EL-213-941501

INTRODUCTION

IDO1 is a heme-containing enzyme that carries out the first and rate-limiting step of tryptophan breakdown along the kynurenine pathway, converting the amino acid, along with related substrates such as serotonin and tryptamine, into N-formylkynurenine. By locally depleting tryptophan and generating kynurenine pathway metabolites, IDO1-expressing dendritic cells, monocytes, and macrophages can slow the proliferation of nearby T cells, push them toward apoptosis, and favor differentiation of regulatory T cells, a mechanism central to peripheral immune tolerance. This same pathway helps prevent autoimmunity and protects the fetus from maternal immune attack during pregnancy, but tumors can co-opt it: IDO1 is expressed by tumor, stromal, or endothelial cells in a large fraction of human cancers, where its immunoregulatory tyrosine motifs sustain its own expression in dendritic cells and help tumors evade immune surveillance, a pattern linked to worse prognosis. IDO1 activity also has antimicrobial and antioxidant roles, restricting the growth of intracellular pathogens by starving them of tryptophan.

PRINCIPLE OF THE ASSAY

This kit uses a sandwich enzyme immunoassay format to measure human IDO1. Antibody specific to human IDO1 is pre-coated onto the microtiter plate wells, where it captures the target from added standards or samples. A biotin-conjugated detection antibody, also specific to human IDO1, is then introduced and binds a second epitope on the captured analyte. Avidin-conjugated horseradish peroxidase (HRP) is subsequently added to each well, linking to the biotin and completing the detection complex. Upon addition of TMB substrate, a colorimetric signal develops exclusively in wells containing human IDO1, the biotin-conjugated antibody, and Avidin-HRP. The enzymatic reaction is stopped by the addition of sulfuric acid stop solution, and absorbance is read at 450 nm ($\pm$ 10 nm). Sample concentrations are determined by comparing well absorbance values against a standard curve.

MATERIALS AND STORAGE

Store kit components at -20°C unless specified otherwise. DO NOT USE past kit expiration date. Some vials contain a small amount of reagents. Spin tubes on pulse setting prior to opening.

Each kit includes:	Units
Pre-Coated Microplate	12 strips x 8 wells
Standard (Lyophilized)	2 vials
Biotinylated Antibody (100×)	120 µL
Streptavidin-HRP (100×)	120 µL
Standard/Sample Diluent Buffer	20 mL
Biotinylated Antibody Diluent	12 mL
HRP Diluent	12 mL
Wash Buffer (25×)	20 mL
TMB Substrate Solution	10 mL
Stop Reagent	6 mL
Plate Covers	2 pieces
<i>Do not mix or substitute reagents with those from other lots.</i>	

MATERIALS AND INSTRUMENTS REQUIRED BUT NOT SUPPLIED

- Precision pipettes calibrated to deliver 5-1000µL
- Multi-channel pipette calibrated to deliver 50-200µL
- Plate shaker
- Disposable tips
- Vortex-Mixer
- Distilled or de-ionized water
- Microplate reader capable of reading 450nm with background subtraction at 620nm

SAFETY PRECAUTIONS

- The test protocol must be followed strictly.
- All reagents containing human material should be handled as if potentially infectious. Operators should wear gloves and protective

clothing when handling any patient sera or serum based products.

- The kit reagents contain antimicrobial agents, acid and 3,3',5,5'-tetramethylbenzidine. Avoid contact with the skin and eyes. Rinse immediately with plenty of water if any contact occurs.
- Any liquid that has been brought into contact with potentially infectious material has to be discarded in a container with a disinfectant. Disposal must be performed in accordance with local regulations.
- Disposal must be performed in accordance with local regulations.
- Only trained laboratory personnel should execute this test.

Human IDO1 ELISA Kit

Sandwich ELISA

Catalog EL-213-941501

PREPARATION OF REAGENTS

Prepare only the appropriate amount of required reagent on the day of use. Store all reagents as per instructions stated on the label.

- 1. Wash Buffer (1X) Preparation: Dilute the 25X wash buffer concentrate 1:25 with double-distilled Water.**
- 2. Detection Reagent (1X) Preparation: Dilute the biotinylated antibody and streptavidin-HRP concentrates 100-fold with Biotinylated Antibody Diluent and HRP Diluent, respectively, immediately before use.**
- 3. Preparation of Calibrators: Prepare calibrators by serial dilution from a 20 down to 0.32 (plus a 0 blank), per the source manual.**

Sol'n ID	Source	Source Vol (μL)	Cal. Diluent (μL)	Final Vol (μL)	Final Conc. (ng/mL)
Std 1	Stock Standard	500	500	1000	20
Std 2	Std 1	500	500	1000	10
Std 3	Std 2	500	500	1000	5
Std 4	Std 3	500	500	1000	2.5
Std 5	Std 4	500	500	1000	1.25
Std 6	Std 5	500	500	1000	0.63
Std 7	Std 6	500	500	1000	0.32
Blank	Std 7	500	500	1000	0

SPECIMEN STORAGE

This kit is compatible with EDTA-plasma, heparin-plasma and serum samples. Samples can be stored at or below -20°C for up to 1 year.

ASSAY PROCEDURE

1. After the kit is equilibrated at room temperature, add 100 μL of Standard Working Buffer (gradually diluted according to the instructions) or 100 μL of sample to each well, and incubate at 37°C for 80 minutes.
2. Discard the liquid in the plate, add 200 μL 1× Wash Buffer to each well, and wash the plate 3 times. After pat it dry against clean absorbent paper, add 100 μL Biotinylated Antibody Working Solution (1×) to each well, incubate at 37°C for 50 minutes.
3. Discard the liquid in the plate, add 200 μL 1× Wash Buffer to each well, and wash the plate 3 times. After pat it dry against clean absorbent paper, add 100 μL 1× Streptavidin-HRP Working Solution to each well, incubate at 37°C for 50 minutes.
4. Discard the liquid in the plate, add 200 μL 1× Wash Buffer to each well, and wash the plate 5 times. After pat it dry against clean absorbent paper, add 90 μL TMB Substrate Solution to each well, incubate at 37°C for 20 minutes in the dark.
5. Add 50 μL Stop Solution to each well, shake plate on a plate shaker for 1 minute to mix. Record the OD at 450 nm immediately, calculation of the results.

CALCULATIONS AND RESULTS

1. Construct a standard curve by plotting the absorbance obtained from each standard against concentration. Use a 4 or 5 parameter curve fit. Alternatively a log-log curve fit may be used.
2. The concentration of the unknowns can be read directly from this standard curve using the absorbance value for each sample.

3. Any sample undiluted or diluted still reading greater than the highest standard should be diluted appropriately and retested. If the samples have been diluted, the concentration determined from the standard curve must be multiplied by the dilution factor.

PERFORMANCE CHARACTERISTICS

Precision: Intra-assay CV < 8%. Inter-assay CV < 10%.

Detection Limit: 0.114 ng/mL

Recovery: Serum (n = 5): 86-97% (avg 92%); EDTA plasma (n = 5): 84-103% (avg 96%); Heparin plasma (n = 5): 82-96% (avg 87%)


Specificity: This assay has high sensitivity and excellent specificity for detection of Human IDO. No significant cross-reactivity or interference between Human IDO and analogues was observed.



This kit employs a sandwich enzyme immunoassay technique to quantify human IDO1 in biological samples.

Human IDO1 ELISA Kit Sandwich ELISA Catalog EL-213-941501

SAMPLE STANDARD CURVE

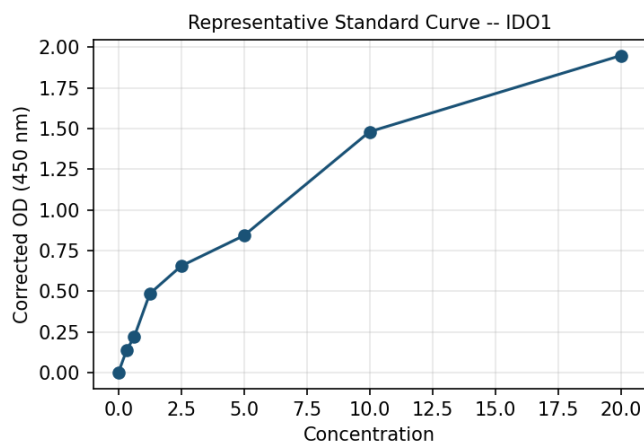

Representative standard curve shown for illustration only. This curve should not be used to calculate unknown sample concentrations -- run a new standard curve with each assay.

ORDERING INFORMATION

Please visit www.affinityimmuno.com to order this product. Visa, Mastercard, AMEX and PayPal are accepted in our online store.

Your order will be processed immediately and you will be notified with a delivery timeframe.